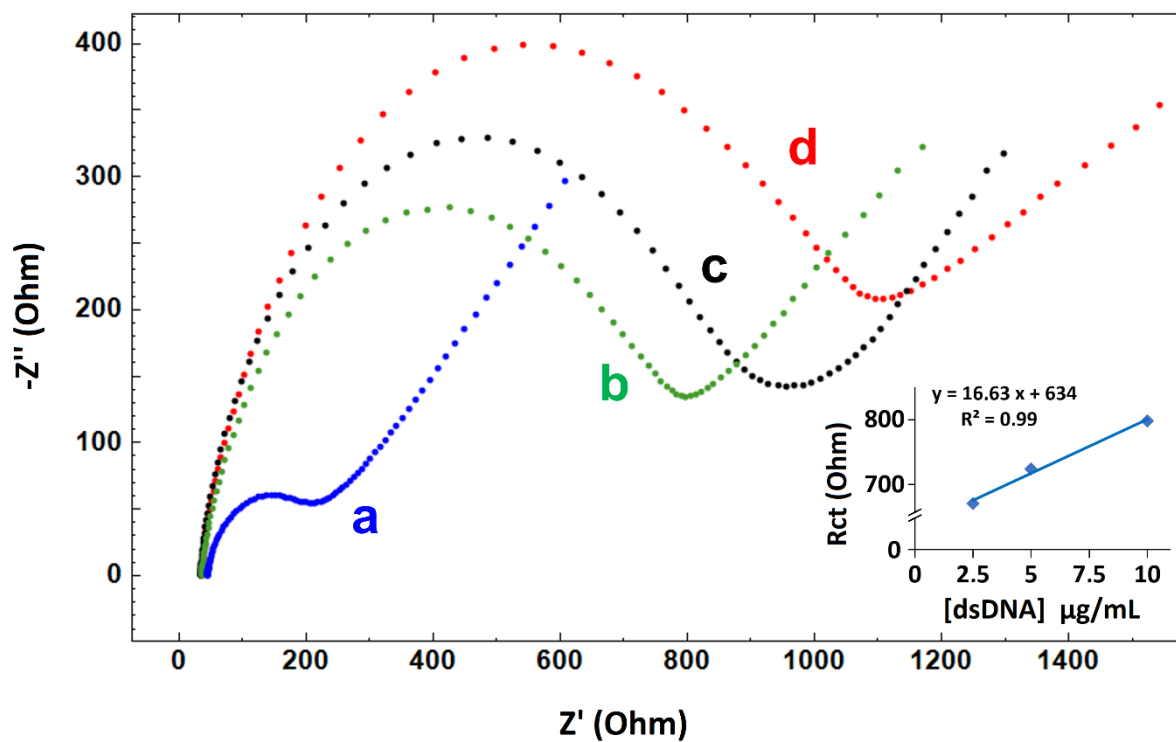


## Supplementary Material

### Fullerene modified single-use electrodes as a convenient biosensor platform for electrochemical monitoring of drug-DNA interaction



**Figure S1.** Nyquist diagrams of (a) f-PGE, (b) 2.5  $\mu\text{g/mL}$ , (c) 5  $\mu\text{g/mL}$ , (d) 10  $\mu\text{g/mL}$  dsDNA immobilized f-PGE. Inset: Calibration plot.